

Accessible Weight Scale for Seated Users

By James I. Johnson
Patrick Tshilenge
Gregory Whitehouse
Team 9

Client: RERC-AMI

Client Contact: Dr. Enderle

University of Connecticut

Bronwell Building, Room 217C

260 Glenbrook Road

Storrs, Connecticut 06269-2247

Phone: (860) 486-5521

1. Optimal Design

Introduction

The clients for the accessible weight scale for seated users all have mobility problems that make it difficult for them to use a standing scale. These clients may want to measure their weight several times a day in order to ensure that they are remaining healthy. The design for the accessible weight scale for seated users will integrate a weight scale into an elevated toilet seat allowing the user to easily and independently measure their weight. The elevated toilet seat design is better than the shower chair design because it is more accessible to the user. Getting in and out of the shower once a day may be difficult for most users. The toilet would be easier to get on and off. The elevated toilet seat was chosen over the regular toilet seat because many users will find it easier to get on and off of the elevated toilet. Also the elevated toilet design can house all of the electronics either within the elevated toilet or within the handheld console without any exposed wires.

The elevated toilet seat scale will have several main components an elevated toilet seat, load cells, a microcontroller, a handheld console, and adjustable and removable foot support. The scale will have handles on the top of the elevated toilet seat to help maintain posture while on the scale and the handheld console will communicate wirelessly with the elevated toilet compartment.

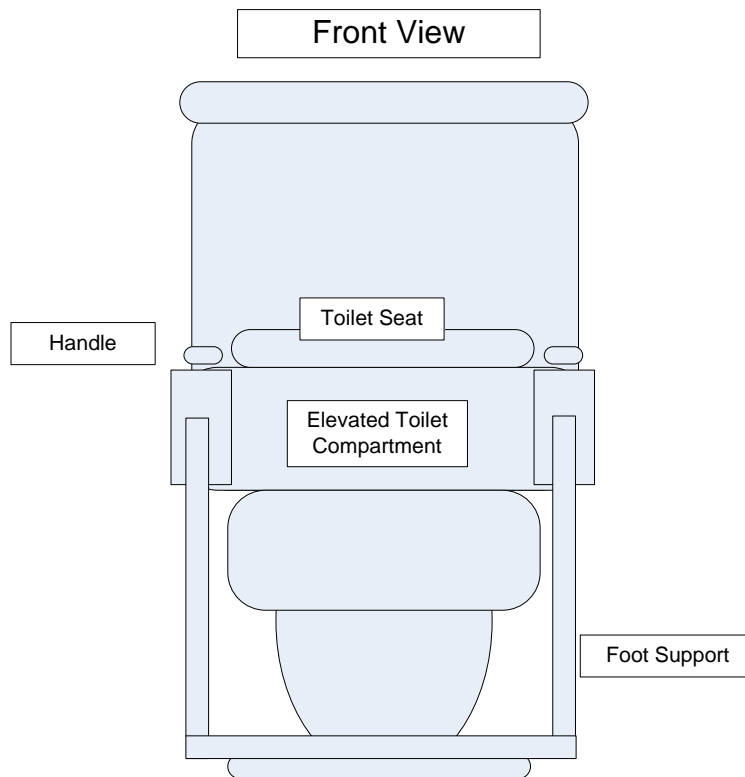


Figure 1 – Optimal Design Elevated Toilet Seat Scale

Figure 1 shows the overall appearance of the elevated toilet seat scale. The scale will have a total capacity of over 500 pounds, an accuracy of 1/5 of a pound, and enough memory to store 25 readings. The scale will also be able to take a measurement in less than 10 seconds and it will provide visual and audio outputs.

The optimal design uses handles on the toilet seat to aid the user in getting on and off the device. If they need additional support to get on the device most handicap accessible stalls in hospitals or clinical settings have mounted grab bars on a nearby wall. The handles will provide some support while the user is on the device since the user can grab onto them when necessary, but they will not obstruct the user in getting on the device.

The adjustable and removable foot support will work similar to the third design. The foot support will be easily adjustable allowing a user with poor fine motor skills to adjust the height of the foot support. By making the foot support adjustable it will be able to support a wide range of users. By making the foot support removable the device will be easier to move from one toilet to another.

The elevated toilet seat serves several purposes. By being elevated it puts the toilet at a similar height to a wheelchair seat allowing the user for easier transfer on and off of the toilet. Similar to other elevated toilet seats currently on the market, this elevated toilet seat will be 5 inches tall. The elevated toilet seat will also house the electronic components as well as acting as the support structure for foot support. A third purpose for the elevated toilet seat is to act as the comfortable seat for the user and mounting surface for the load cells.

Three load cells will be used to measure the weight of the user. They will be loaded on the bottom of the elevated toilet seat similar to the third design. The load cells will measure the compression force applied by the user on the elevated toilet seat and send the signal through wires to the printed circuit board (PCB) inside the elevated toilet seat. A waterproof plastic will be used to cover the load cells to prevent them from becoming wet.

Also incorporated into the elevated toilet seat compartment will be the microcontroller, which will be responsible for converting the signal from the load cells into a weight measurement that can be stored in the microcontroller and outputted in both kilograms and pounds. These outputs will be sent to the handheld console via a wireless transmitter.

The purpose of the handheld console is to act as the user interface for the accessible weight scale for seated users. The user can use this component to take a measurement or to view past readings. The handheld console will come with two Velcro strips. One side will be attached to the back of the handheld console and the other side can be attached to the toilet or the wall or any other place in the bathroom that is convenient for the user. This will allow the user to mount the handheld console wherever they choose when they choose to mount it. It will also allow them to easily take it from the mounting and hold it in their hand for easy reading and convenient inputting of values.

Figure 2 shows a block diagram of the operation procedure for the accessible weight scale for seated users below. The user inputs are shown in rectangles with rounded edges and the

actions completed by the accessible weight scale are shown in rectangular boxes with sharp edges.

Prior to using the device for the first time the user will have to turn the device on and press the “Tare” button on the handheld console. Pressing this button will cause the scale to take a measurement without the user on the device. This measurement will be stored in the microcontroller as the weight of the scale alone. This weight will be subtracted from the user’s weight when a measurement is taken so that the weight outputted by the device is the weight of the user alone. To provide the most accurate measurement the user could tare the device prior to every use, but it is not necessary if a small amount of error is allowable.

To operate the device the user will pick up the handheld console and switch the analog switch to the “ON” position. Next the liquid-crystal display (LCD) screen interface will display the message “Please be seated on the scale and press the measure button when ready.” This prompt will also be given in the form of audio output so that the user with impaired vision will receive the prompt as well. The user now has two choices. He or she can get on the scale and take a measurement or they can view past measurements by pressing the scroll up or down key. If it is more convenient for the user, the user can get on the device prior to turning it on as well.

To take a new measurement the user will get on the scale and press the “Measure” button. At this point the sensors under the seat will send the reading to the microprocessor, which will subtract the current weight from the weight of the scale. This will be the measurement of the user’s weight, which will be converted into kilograms and pounds, stored in the memory, and displayed for the user on the LCD screen as well as the audio output through the speaker. The user now has the option of turning off the device or viewing past measurements.

The user can scroll through past measurements by pressing the up or down arrow on the user interface. These weights will be displayed in both kilograms and pounds. Figure 2 shows the block diagram of the process outlined above.

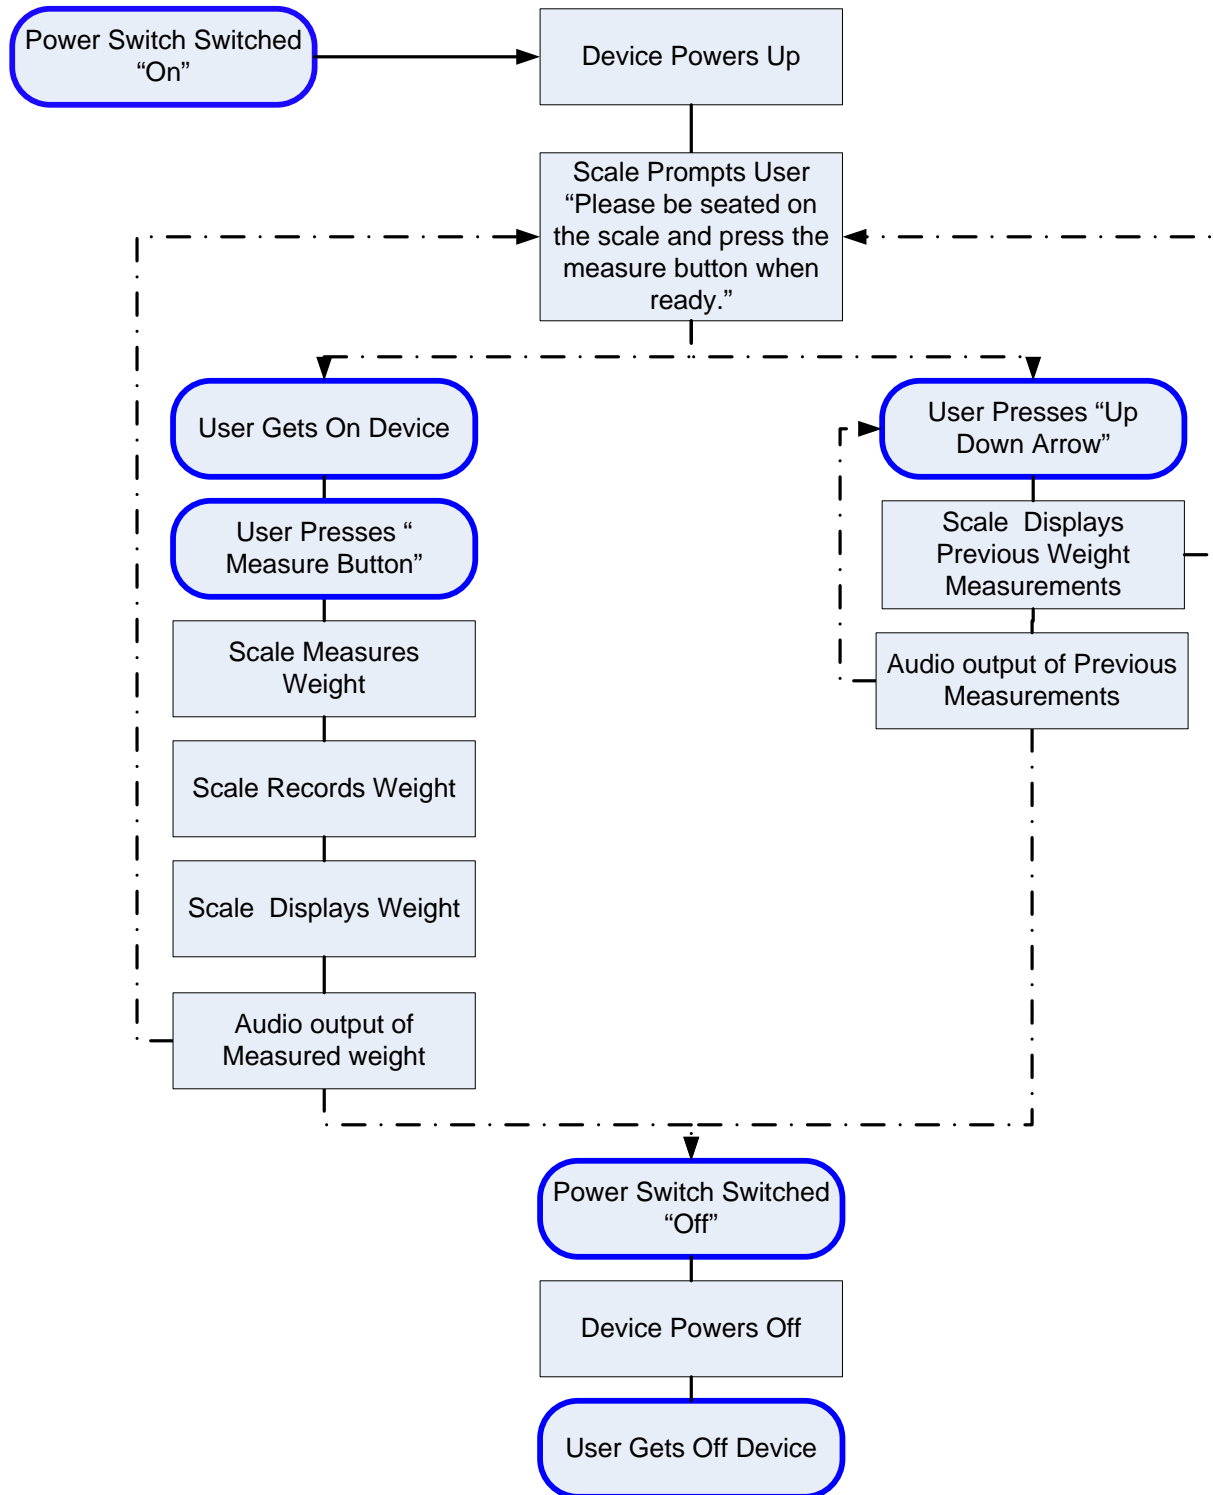


Figure 2 – Block Diagram of Operation Procedure

There are several differences between this operation procedure and the operation procedure of the third alternative design. The third alternative design turned on as soon as the user gets on the device and required the users to identify themselves in order to be able to store readings for five different users. The optimal design will be switched on using the toggle switch

on the handheld console similar to design 1 and 2. This decision was made because of the possibility that the user does not live alone. If the user lives with children and the device turns on automatically the children may take measurements when not supposed to. Also the battery life for the scale is a concern. It would be best if the user did not have to change the batteries often. By having the scale turn on whenever the user gets on the toilet, the scale will use battery life whether or not the user is trying to take a reading. By having the scale only turn on when the user wants to take a reading, the scale will conserve as much battery life as possible.

The other operational procedure difference is the step of inputting the user identification number. The decision to exclude the capability of measuring multiple users was made because in a nursing home or hospital where there may be multiple users, the weight measurements would be recorded. Also the scale only had the capability to measure up to five users, which would not be enough for most clinical settings. Also it may be difficult for users to remember their user number and in most household settings it would not be necessary. Future generations of the accessible weight scale for seated users may allow for multiple users, but the first generation of the product will not.

1.2 Subunits

Load cells

The function of the load cells is to measure the compression force of the user sitting on the toilet seat. This compression force is changed into an electrical signal which is then sent to the elevated toilet compartment via wires, and input into the A/D conversion ports on the microprocessor for conversion of the analog signal to a digital signal. Most load cells are based off of traditional strain gauges, and utilize strain gauges to provide accurate measurements. The strain gauge has a thin metallic foil that is bonded to a dielectric layer, which transmits the electrical signal using induction. This involves the electrically charged film to create an additional electrical charge, which is sensed by the strain gauge. When a force is applied to the strain gauge, the foil is deformed causing a change in its electrical resistance. A Wheatstone Bridge then measures the changes in resistance, and relates this value to the gauge factor, where $GF = (\Delta R/R)/(\Delta L/L)$. A figure showing the related forces and dimensions of strain is shown below:

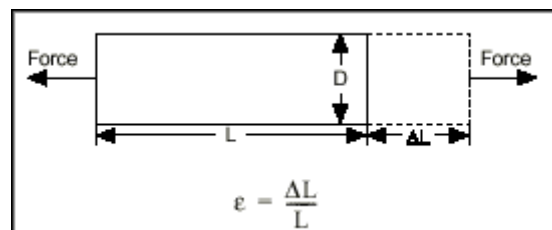


Figure 3 – Strain Specification

The Wheatstone Bridge consists of four resistive arms with a voltage excitation source. When the excitation voltage is applied across the bridge the output voltage will equal the following equation:

$$V_O = \left[\frac{R_3}{R_3 + R_4} - \frac{R_2}{R_1 + R_2} \right] \cdot V_{EX} \quad [1]$$

The output voltage can then be used to calculate the applied force onto the strain gauge. The output voltages of strain gauges are usually quite small; therefore, the output signal will have to be amplified to boost the signal level for an increase of measurement resolution and improved signal to noise ratios. The amplification will also allow for the microprocessor to receive the appropriate minimum current for A/D conversion of the signal. Also, as with many electronics, there will be noise that can couple to the strain gauges. Therefore, a low-pass filter will have to be implemented to remove the high frequency noise associated with the electronics and environment.

In order to function correctly, the strain gauge must be mounted to a strain element using an adhesive due to the delicacy of the thin piece of wire within the gauge. The strain gauges that are intended for use in the project utilize a simple beam mounting configuration. This configuration, along with the proper adhesive, should allow for high accuracy and little error in the calculations. The strain gauge and element will have to be housed in either a laminate material or metal casing in order to prevent shock to the load cell, as well as adequate prevention of contact with liquids.

There are numerous different load cells available on the market, but for the design project the SMD Sensors S400 Button Cell load cell has been chosen in order to provide optimal functionality while being relatively cost-effective. An initial search for load cells resulted in many high capacity rated load cells that were very expensive. The S400 Button Cell, rated at a capacity of 500 pounds, has a cost of \$350 per load cell. The group intends to implement three load cells for the design and manufacture of the device. Although, three of the S400 Button Cells will be costly, they will be excellent in meeting the weight specifications and requirements for the device. Three of the load cells, all rated at 500 pounds capacity, will provide optimum weight measuring capacity and accuracy. Also, the S400 Button Cells are quite small and have a low-profile appearance, which will allow for the placement of the load cells on the bottom of the elevated toilet compartment; thereby, mimicking the actual stops or cushions on the underside of a toilet seat. As previously mentioned, proper adhesive will have to be used to mount the load cells to the bottom of the elevated toilet compartment, and small circular stops will have to be placed on the top, flat portion of the toilet bowl where the load cells will undergo compression when the user is seated on the seat. This will result in unwanted slippage of the elevated toilet compartment, and consequently the load cells, when the toilet seat is down and weighing is taking place. It will also provide accurate calibration of the load cells when the user tares the weight scale. A picture of the load cell, its isometric view, and its dimensions are shown on the following page, and its related specifications are attached as appendix A:



Figure 4 – S400 Button Cell Load Cell

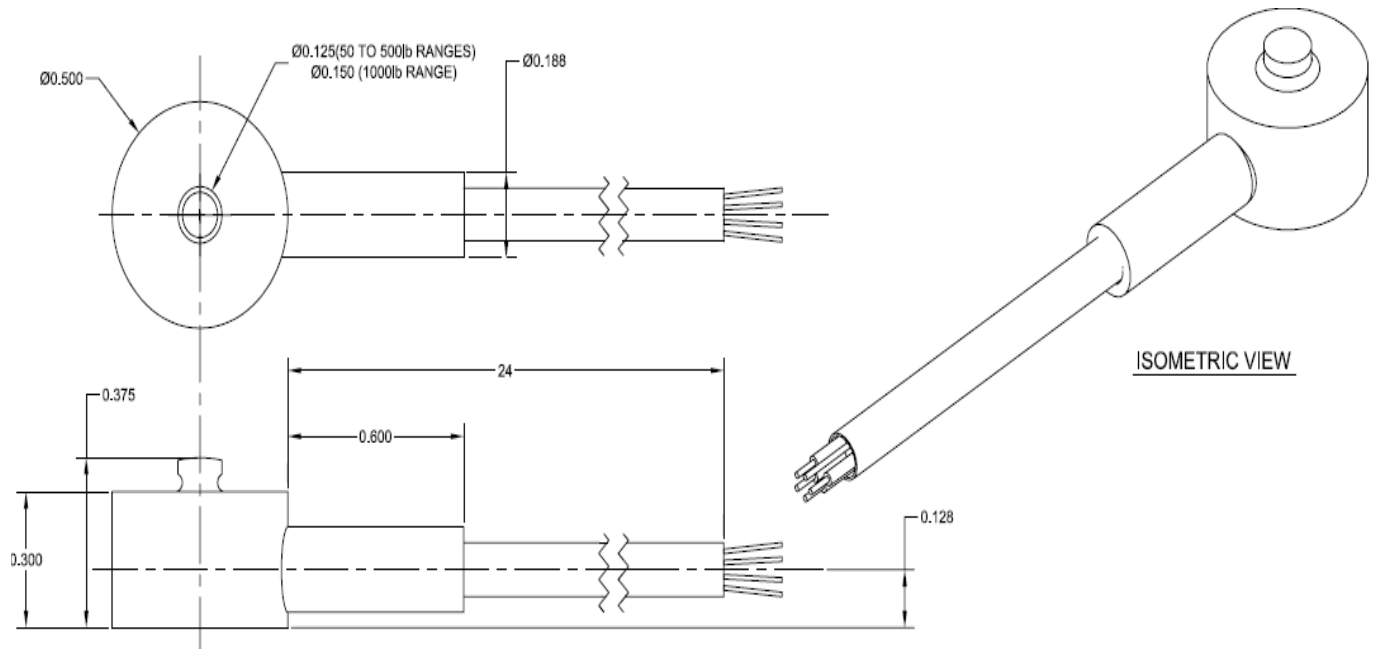


Figure 5 – S400 Button Cell Isometric View and Dimensions [2]

A very significant part of the optimal design, as with all of the former designs, especially concerning electronics and electrical components, is keeping the elevated toilet seat scale as waterproof as possible. This is quite necessary when considering the mounting and placements of the three load cells. As previously mentioned, the load cells will be mounted to the bottom of the elevated toilet compartment. They will have to be fastened, with waterproof adhesive and sealant, into circular holes that meet the radiuses of the button cells. This setup will allow for the button parts of the load cells to face down and undergo the compression of the user sitting on the elevated toilet seat, which will then result in the weight measurement. The S400 Button Cells will have to be covered with a thin plastic film in order to keep water or condensation from contacting the load cells. The plastic covering will have to be thin enough to allow for accurate load cell measurements, while not disrupting the distribution of forces when the user is sitting on the toilet seat. The shielded wires from the load cells will enter directly into the elevated toilet compartment for input into the A/D pins on the microcontroller, and the compartment will ultimately be the housing of the electronics and electrical components.

Elevated Toilet Seat Component

The elevated toilet seat will be mostly constructed in the machine shop. It will consist of several different parts. The elevated toilet seat will have a normal toilet seat with hinged cover for the user to comfortably sit on. This will be attached as a normal toilet seat would with a hinge and a toilet seat cover. The toilet seat that will be purchased for this design is shown below in Figure 6. It comes with non-corrosive hardware to attach the seat on top of the rest of the device. This toilet seat was chosen because it is made of wood and can support an overweight person. This toilet is not specifically made for an obese person and therefore may not be comfortable for a person who is 500+ pounds, but it could support their weight. There are toilet seats that are designed for a person who is morbidly obese, but since none of the theoretical clients for this project is morbidly obese, a normal toilet seat was chosen for maximum comfort of the theoretical users.



Figure 6 – Bemis 500PRO Round Wood Toilet Seat

Figure 7 below is a diagram of how the elevated toilet seat will appear. The prototype for this device will incorporate all of the electrical components inside the elevated toilet. These components can be accessed by removing the top panel of the elevated toilet using a screwdriver. The inside of the panel will be lined with weather stripping to prevent water from leaking in when the panel is securely fastened on the device and the device is in use. The elevated toilet encasing will be made of thick hard plastic encasement with high tensile strength and bend modulus. The encasement will have a hole in the middle the same size as the Bemis toilet seat. The sides of the encasement will extend farther than the sides of the toilet seat. The handles will be screwed into the top of the encasement and the foot support will fit into slots in the extended portion of the encasement. As described above the load cells will be attached to the bottom of the encasement in between the encasement and the toilet.

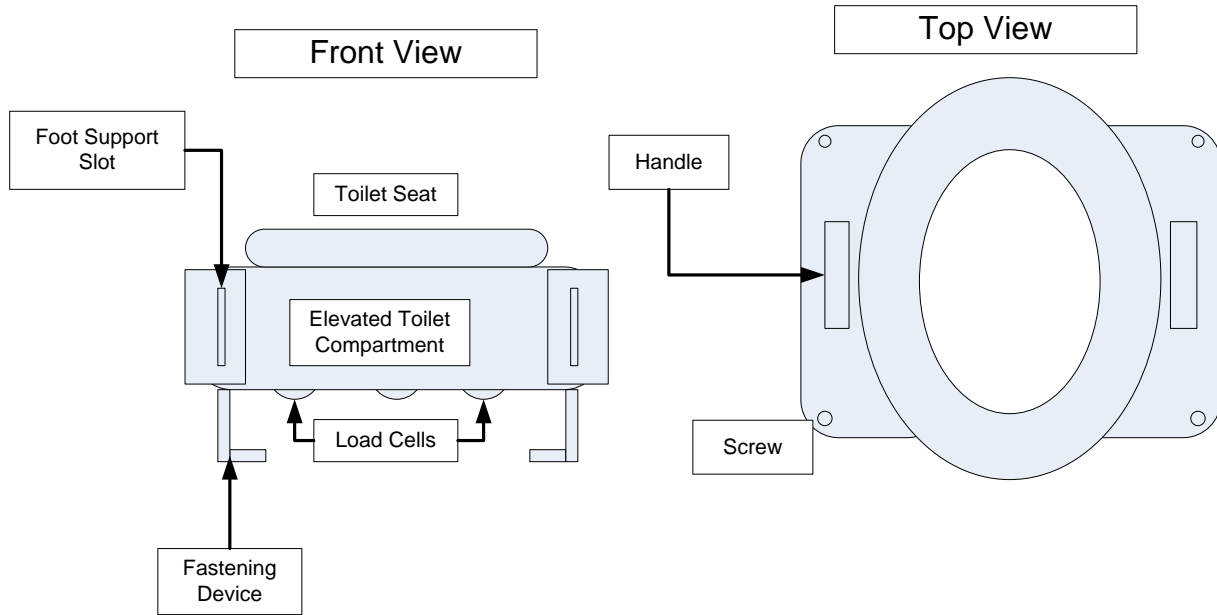


Figure 7 – Elevated Toilet Seat Design

The encasement will be fastened to the sides of the toilet using four clamp mechanisms located at the four corners of the elevated toilet seat. The fastening mechanism is shown below in Figure 8. The rubber stopper will act as the interface between the fastening mechanism and the toilet. The rubber stopper will be attached to a swivel end so that its surface can change its angle to match the curvature of the toilet it is coming into contact with. The fastening device will hold the seat in place without affecting the readings from the load cells. The fastening mechanism will be attached to the toilet seat using a two screws and a metal plate. The handle will go through a hole in the screw and will be turned to extend the rubber stopper toward the toilet seat or retract it from the toilet seat.

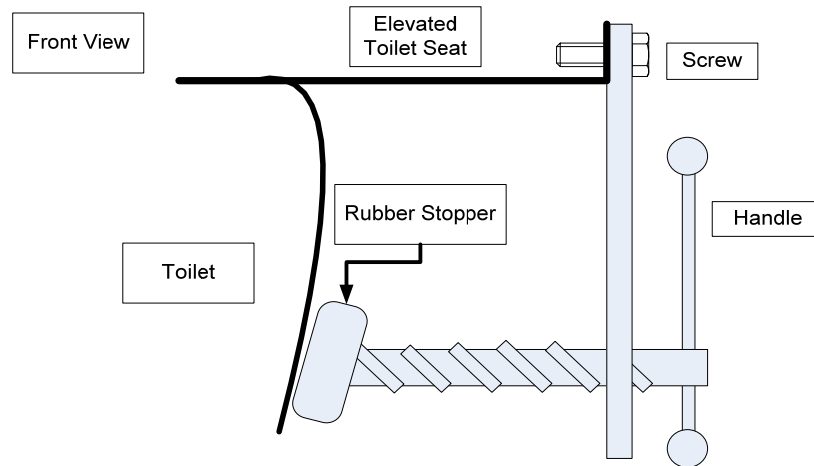


Figure 8 – Fastening Mechanism for Elevated Toilet Seat

The elevated toilet seat will contain the “guts” of the device, including the printed circuit board (PCB) and related electrical components, batteries, wires, and wireless transmitter that will communicate to the mounted display. The bottom panel of the elevated toilet seat will be removable to allow for easy access to the circuit within; thereby, allowing for necessary modifications or repairs to the electrical circuit board or PCB. This part of the electrical component compartment will not be accessed by the user, but by an individual who is familiar with electronics and electrical components in the event that a modification or repair is needed. It will also need to be lined with a weather stripping in order to prevent water from entering into the electrical component compartment. There will also be another easily accessible compartment on the front of the elevated toilet seat compartment that will allow the user to easily change the batteries when necessary. This accessible battery compartment will also need to be lined with weather stripping in order to prevent liquid or condensation from entering the compartment and subsequently damaging the batteries. An example of the circuit schematic for the power supply to the microcontroller is shown and explained on the following page:

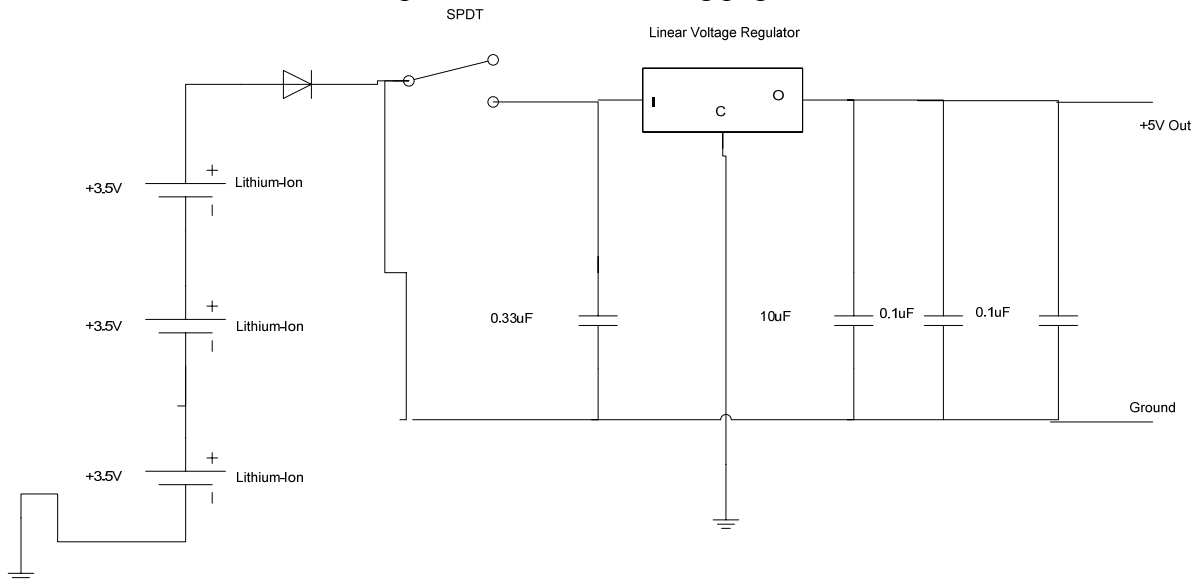


Figure 9 – Example of Power Supply to PIC Circuit

Three lithium-ion batteries will be wired in series and used as the power supply for the device. They are rated at approximately 3.5V a piece; therefore, a voltage of about 11.5V will be output from the three batteries mimicking a 12V DC power supply, which should be adequate in meeting the power requirements for the device. A current limiting diode will be placed after the batteries and before the switch for prevention of electrical damage to the batteries. A single-pull-double-throw switch (SPDT) will be placed after the diode in order to function as a disconnection of power to the linear regulator. For input into the voltage regulator, a 0.33uF capacitor will be necessary to filter out unwanted spikes or noise in the signal that could occur after the switching. After the linear voltage regulator will be a 10uF capacitor that will filter out any more unwanted voltage spikes that could occur after the switching and power up. Also, the input and output pins of the linear voltage regulator will have to be grounded to a common ground to provide the true functionality of the regulator, thereby supplying the desired 5V output. Finally, two 0.1uF capacitors will be placed after the 10uF and will be connected to the power and ground pins of the electrical components to filter out additional noise and voltage

spikes. One decoupling capacitor could possibly be used to filter out all of the noise and voltage spikes as aforementioned; however implementation can most easily be realized during the testing of the circuit(s) on a protoboard. The circuit will be necessary and will work to down regulate the 11.5V from the lithium-ion batteries to provide the 5V output necessary for supply to the microcontroller and electrical components.

All of the electrical components included in the elevated toilet compartment will need to be tested on a protoboard prior to ordering the printed circuit board so that the group is ensured the correct PCB schematic is sent. A standard smoke test will inevitably be performed when first powering on the electronics to make sure that all of the electrical components are functioning correctly, and will function correctly when eventually connected to the PCB. A digital multi-meter will be used to check voltages, currents, and resistances throughout the protoboard to make sure that they meet the specifications of the various chips and linear voltage regulator, and so that there are no short circuits throughout the circuit.

The structural integrity of the elevated toilet seat will be tested similarly to the toilet seat in the first alternative design. The device will be tested with varying weights to ensure that the device can hold over 500 pounds and that the load cells will be able to measure that weight accurately and efficiently.

Handles

The handrails from the first and third alternative designs will not be used in the optimal design. The group has decided that there are significant issues with stabilizing the handrails from those designs and keeping them from obstructing the user while getting on the device or while sitting on the device. In order to keep the design as simple and easy to use as possible the handrails will be replaced by two handles fastened to the top of the elevated toilet compartment as shown in Figure 7 above. These handles will give the user something to grab onto while getting on the device without being in the way of the user while they are on the device. The handles will not be adjustable, but they will not extend any higher off of the elevated toilet compartment than necessary to meet the design specifications put forth by the Americans with Disabilities Act (ADA). The handles will be made of an aluminum alloy with a rubber covering to maximize user comfort and grip. It would also be beneficial for the user to use an ADA approved grab bar in conjunction with this device if extra transfer support is needed.

The handles will apply a vertical downward force on the toilet seat. When in use the weight applied to the handrails will be incorporated with the rest of the weight of the user. The vertical resistance of the hand rail will be tested by applying 250 lbs on each hand support. For the lateral resistance test a hook will be attached to 250 lbs and it will be hanged from the side of the handles in order to ensure compliance with the Americans with Disabilities Act (ADA) requirements.

Foot Support

The function of the foot support is to keep the user's feet off the ground. The weight applied to the foot support is distributed to the elevated toilet seat. This will ensure that all of the user's weight is distributed onto the elevated toilet seat and incorporated into the measurement.

Figure 10 below shows a side view of one of the leg support sides. Figure 11 below shows the foot support plate that will fit into the adjustable notches on the sides of the leg support.

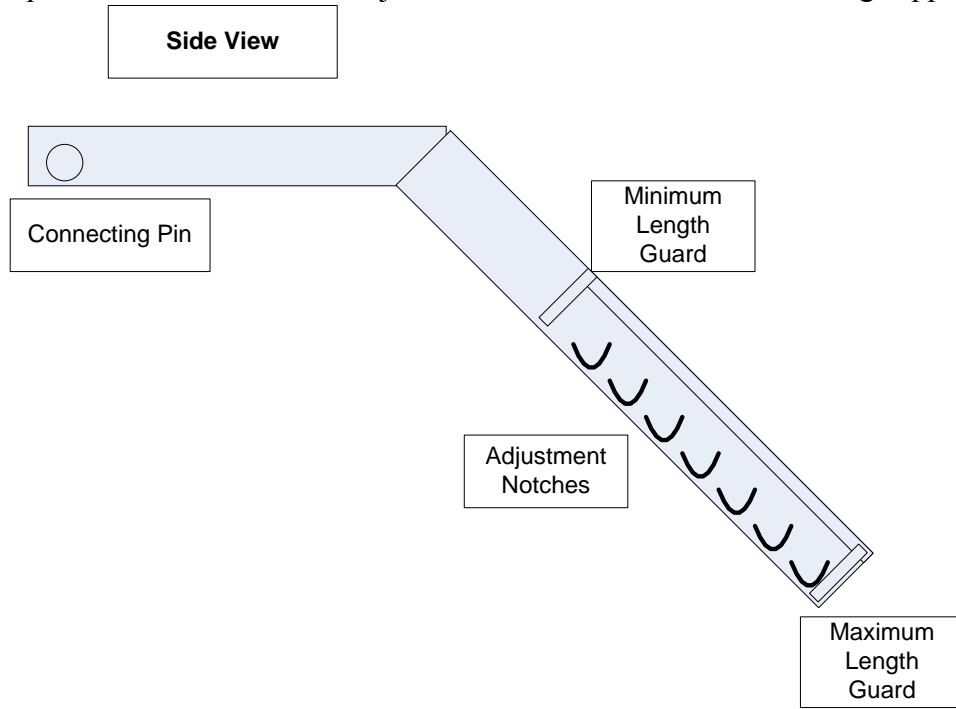


Figure 10 - Side View of Foot Support

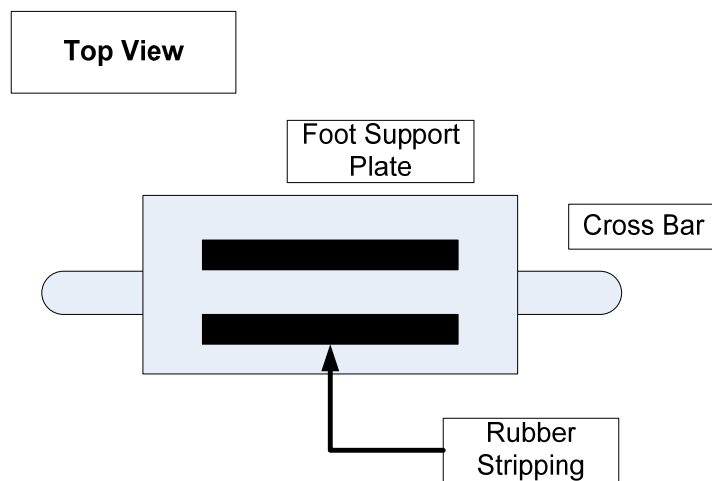


Figure 11 - Top View of Foot Support plate

The foot support will be adjustable and detachable for the user's convenience. The foot support will be adjustable using the adjustment notches. The user will rest their feet on the foot

support plate. The foot support plate will be welded to a bar that extends a few inches past the plate. The ends of the bars will rest inside the adjustment notches. In order to increase or decrease the length of the foot support the user simply move the foot support plate up or down onto a different adjustment notch. In order to make sure that the foot support plate does not fall out entirely there will be guards at the top, bottom and along the side of the foot support to prevent the user from removing the plate entirely while the foot support is in. This mechanism for adjustment is different from the third alternative design that used a spring pin mechanism to adjust the length of the foot support. This design for adjusting the height of the foot support will be easier for a user with poor fine motor skills.

The foot support will fit into the slots in the front of the elevated compartment of the elevated toilet. These slots will be separate from where the electrical components are housed. Once the foot support is slid into the slot all of the way a pin will be placed through the hole at the top end of the foot support to hold the foot support in place. The pin will be made of the same aluminum alloy as the foot support and will be relatively thick to make sure that it can support the weight of the foot support without breaking.

All these components will be made of an aluminum alloy to reduce the weight of the foot support and resist corrosion. Also to add comfort and traction for the feet of the user two rubber strips will be glued to the surface of the metal plate using a plastic adhesive.

The strength of the foot support will be tested by applying 550 lbs on the support. The device should be able to withstand a weight of up to 500 lbs. This test is essential to avoid any injury to the user and or damage to the device because the 500 lb user might stand on the foot support while getting on the device.

Microcontroller

The microcontroller is responsible for converting the electrical signal from the load cells into a weight measurement given in kilograms (Kg) and pounds (lbs). It is also responsible for storing the data of the collected weight measurements, and incorporating a wireless transmitter and receiver for communication between devices.

The PIC18F6723 microcontroller, made by the Microchip Corporation, will be used for the accessible weight scale for seated users project, and will be used in the elevated toilet compartment. The PIC18F6723 microcontroller was chosen for the project for numerous, various reasons. A main reason is that it has 128 kilobytes of program memory as well as 3936 bytes of data memory, which will be essential for storing multiple readings taken from numerous weight measurements. It also has twelve onboard, 12 bit analog-to-digital module inputs, which is an amount that is higher than what is needed for the project, the device only requiring three inputs for the load sensors; however, if more load sensors were later required for some reason, then the microcontroller would easily allow for the implementation of those sensors. A USART output pin will be used to transmit serial communications via a wireless transmitter to the microcontroller within the handheld console.

For the optimal design of the project, it was determined that a second microcontroller would need to be implemented in order to incorporate a wireless handheld console. Therefore,

the PIC16F874A microcontroller was chosen due to a familiarity with programming, debugging, and utilization of this microcontroller in past projects. The LCD screen and buttons will be connected to the input I/O pins of the microcontroller, and the wireless receiver will be connected to one of the USART input pins for serial communication with the elevated toilet compartment.

As just mentioned, the PIC microcontroller employs USART serial communications, and it can allow for access to a computer through a serial port when a proper RS232 chip is used. The Microchip MPLAB Integrated Developer's Environment can also be used for the programming and debugging of the PIC microcontroller. It is also capable of parallel communications (PSP), thereby allowing for compatibility with peripheral devices and wireless applications. Furthermore, both the PIC18F6723 and PIC16F874A are stocked with Microchip's nanowatt technology, which limits power dissipation while increasing the electrical life when the PIC and device are operating on battery power; this will be useful for the group's device, which will be operating solely on battery power.

As previously stated, the analog-to-digital conversion ports will be used for the output signals of the load sensors, in order to convert the electrical signals into actual values of weight, in pounds and kilograms, for display on the LCD screen. There are in-circuit-debugger (ICD) ports which will be used for the programming and debugging of the microcontroller. The programming and debugging can be done using the MPLAB IDE in conjunction with the Microchip ICD 2 or PICSTART Plus. Programming will either be done in the assembly language (ASL) or C++ language. It is much easier to program in C++, mainly due to the simpler use of loops in C++ in comparison to the numerous bundles of programming in ASL. However, each programming language can be converted to the other for greater ease of programming. Testing the microcontroller will be done by setting up a protoboard circuit that has a power supply and telephone type data connect, which will plug into the Microchip ICD 2 for debugging and eventual programming. Showing that the microcontroller is actually functioning will require the use of an oscilloscope and probe, which should show a 5V peak to peak sinusoidal wave assuming that the protoboard is wired correctly. The following figures are connection diagrams for the PIC18F6723 microcontroller and the PIC16F874A microcontroller, showing certain pin connections for supply voltages, grounds, A/D conversions, data output, and digital output:

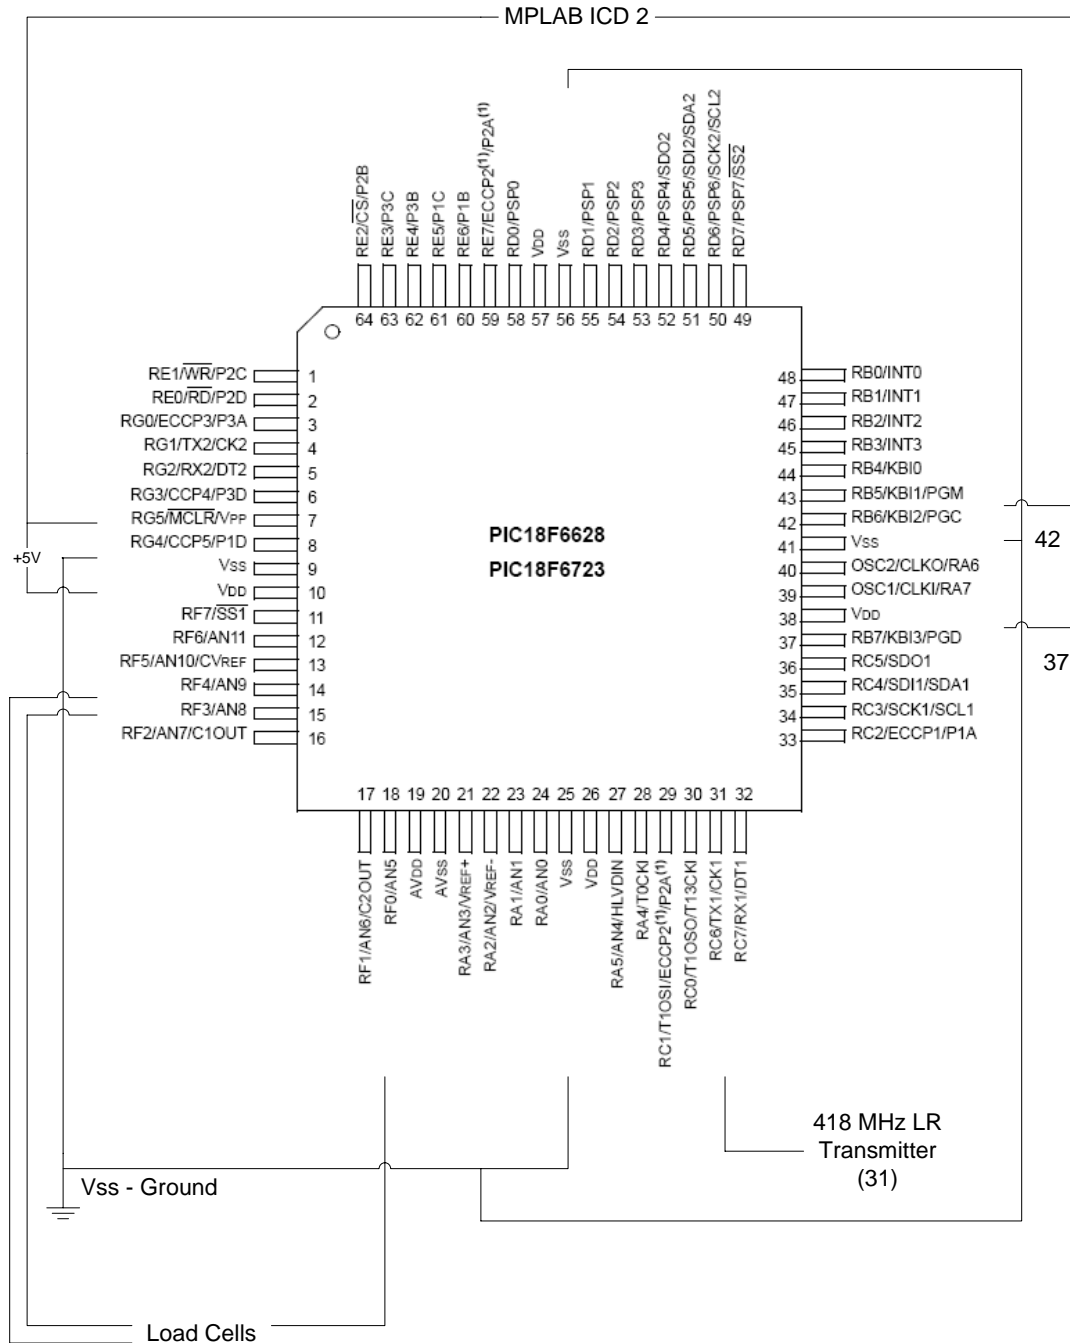


Figure 12 – PIC18F6723 Connection Diagram

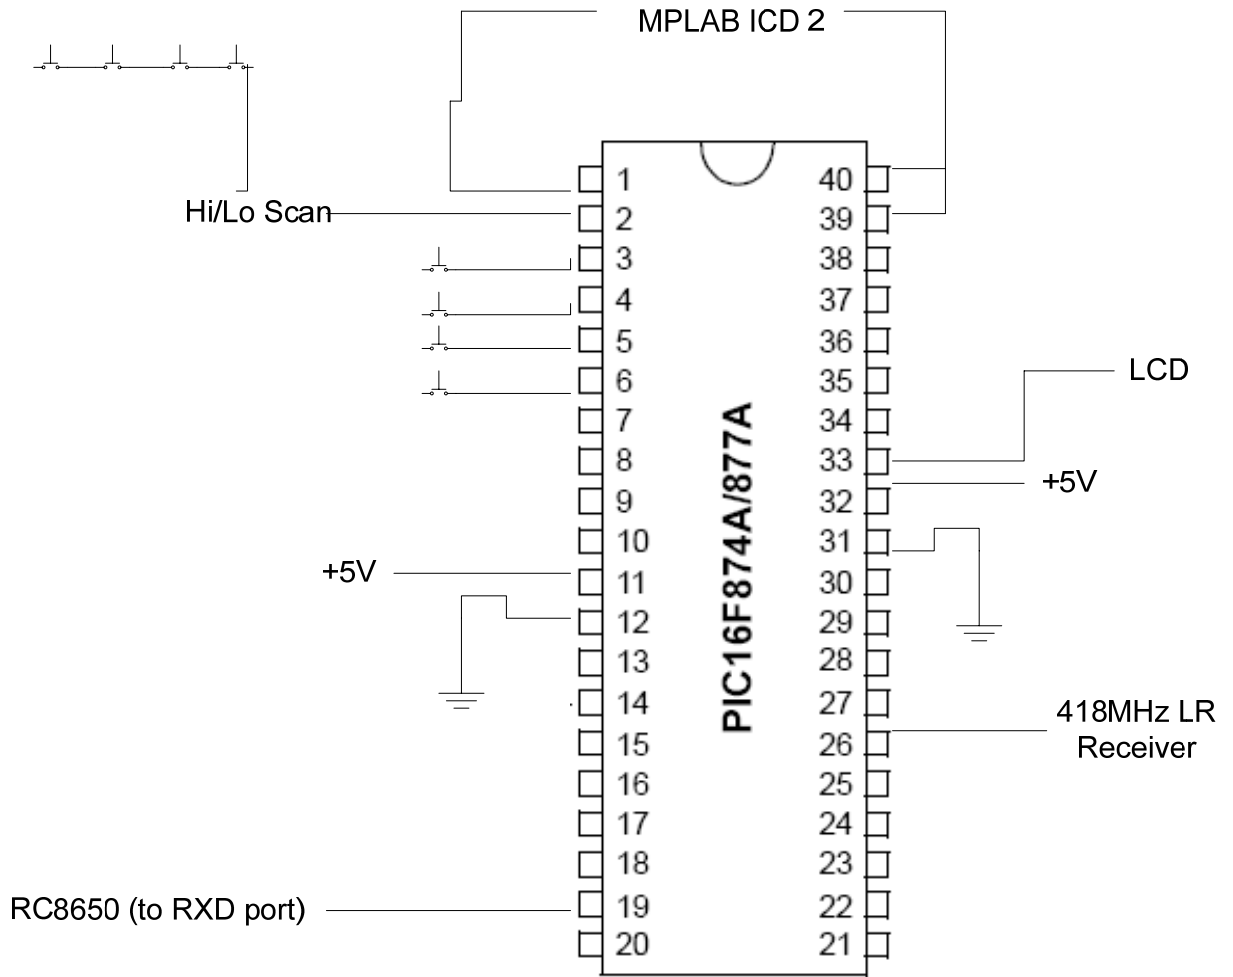


Figure 13 – PIC16F874A Connection Diagram

The programming will accomplish acknowledgment of button pressing by setting a low bit and a high bit. All of the buttons will remain low when they are not pressed, yet, when one of the buttons is pressed, the microcontroller will sense the pulse and acknowledge the button that is being pressed. Acknowledgement of button pressing can also be accomplished by using separate digital I/O (input/output) ports for the input of buttons, and using internal interrupts within the programming to sense which button was pressed. In Figure 13, buttons are shown for both situations, with the separate digital inputted buttons wired into pins 3, 4, 5, and 6. Examples of assembly language source code for A/D conversion, initialization of an LCD, and button pressing are included as appendices B, C, and D respectively. The source code was programmed to a PIC16F874A on a student education board.

Handheld Console

The handheld console from the second alternative design was chosen for the optimal design. Since the optimal design does not have handrails like the third alternative design the mounted display would not work. Also it is more convenient for the user to decide how and where they would like to mount the display. The handheld console is wireless to reduce the

number of wires that are exposed to the environment and also for more convenient mounting. Figure 14 below shows how the handheld console will look for the optimal design.

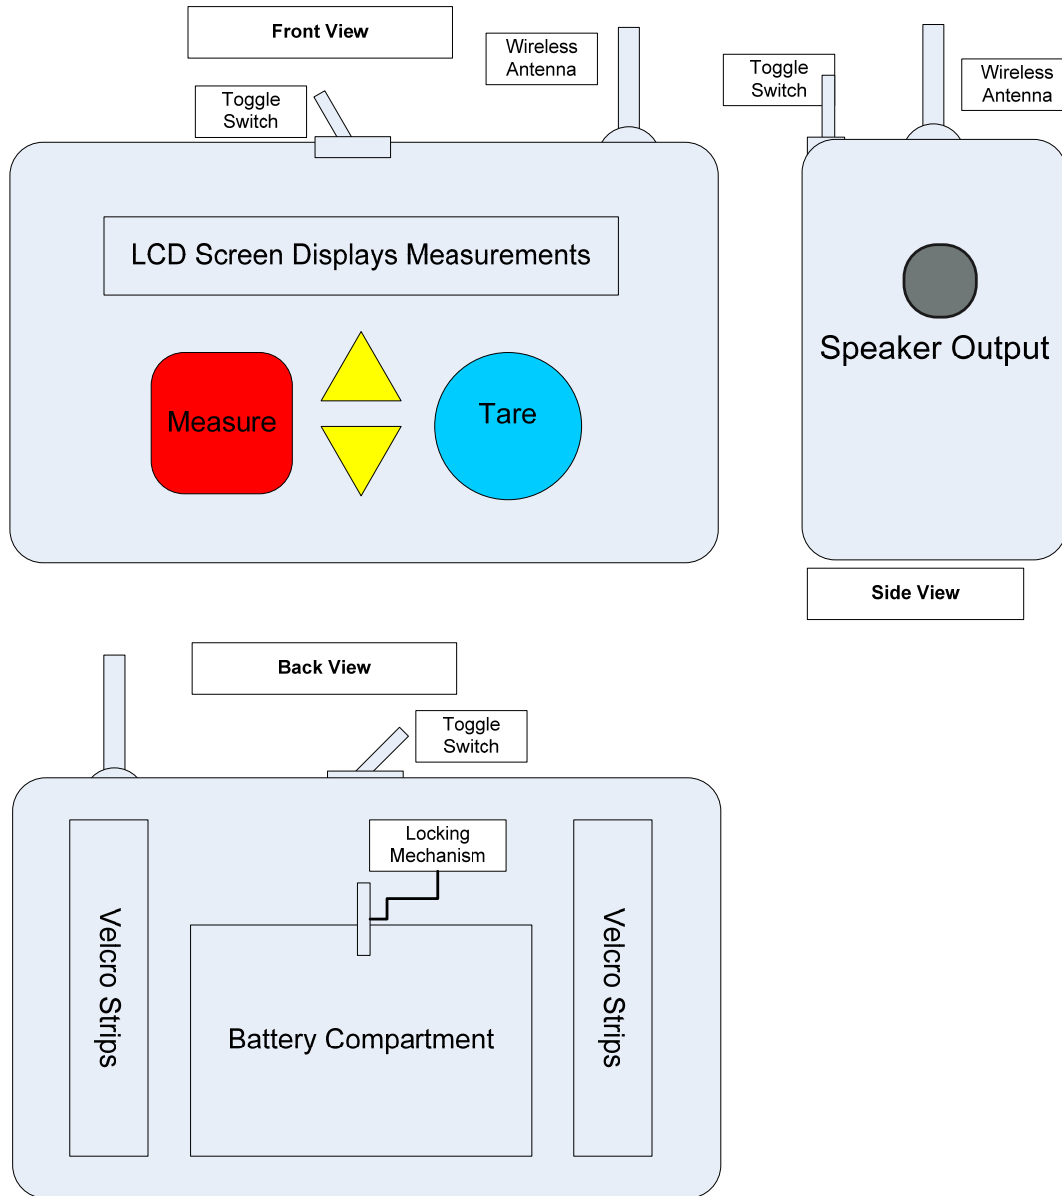


Figure 14 - Handheld Console

The handheld console functions as the user interface for the device. It contains a toggle switch on the top of the console to allow the user to easily turn the device on and off. It will also contain a “Tare” button that will allow the user to tare the device prior to getting onto the scale. It will contain a “Measure” button that will allow the user to easily take a measurement once seated on the scale. There will be a scroll up and down button that will allow the user to scroll through previous readings. There will be a liquid crystal display (LCD) screen that will have characters about half of an inch in height. For audio output the user interface will contain a speaker and text to speech device. The handheld console will be connected to the electrical component compartment via wireless transmission and serial communication.

The handheld console will be connected to the other electrical components housed within the elevated toilet seat via wireless transmission and serial communication. The handheld console will take 9 V batteries that will be easily accessible from the back of the console. A linear voltage regulator circuit will have to be implemented in order to down regulate the 9 V battery output to a 5 V LCD input. The LM317L linear voltage regulator manufactured by ON Semiconductor Corporation will be used as the linear voltage regulator for 5V input into the LCD screen. These voltage regulators have a variable voltage output of 1.2V to 37V, which will incorporate the needed 5V output and input into the LCD, and will work well considering the use of 9V battery power supply. The current output for the LM317L is in excess of 100mA, which is not too high of a current, but will still make it necessary to put a current limiting diode in series with the 9V battery in order to prevent backflow of current, which could damage the battery and possibly other electrical components (shown in Figure 17). A circuit diagram of the external components wired to the LM317L is shown below, and will be wired as so for the design of the device:

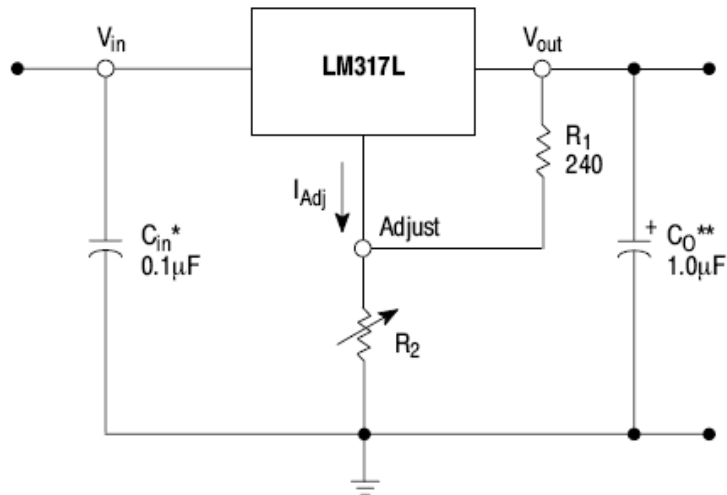


Figure 15 – LM317L Linear Regulator Circuit Setup [3]

The LCD that the design group intends to use is the LCM-S01602DSR/D manufactured by Lumex Inc., and a picture of the LCD screen is shown below:



Figure 16 – LCM-S01602DSR/D [4]

The LCM-S01602DSR/D screen, shown above, is ideal for the group’s design for a few reasons. The first reason is that it has sixteen characters X two lines, which will be useful when

sending messages to the users from the microcontroller, as well as when displaying the weight measurement readings. Another reason is that it has a large viewing area with a dimension of 99 X 24 mm, providing a fairly big view to the users. The LCD also has a character size of 4.84 X 9.63 mm, which will make it easier for any user with vision impairments to read the screen. It has a wide viewing angle, which will easily compensate for viewing if a user is holding the handheld console at an angle. The backlight on the LCD will make it easier to read in dimly lit settings. Lumex states that the LCD has low power consumption with long operational life and that will be vital to the accessible weight scale, as batteries will be used and replacing them often is not desired. It must also have a voltage input of 5V and a 12mA current. A schematic for the power supply to the LCD screen is shown below:

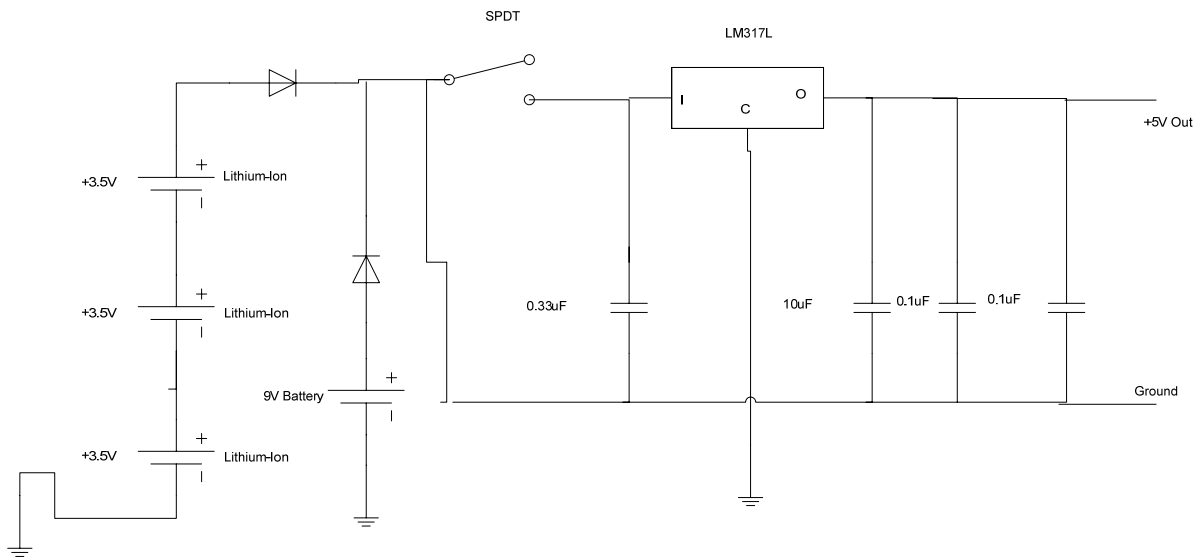


Figure 17 – Example of Power Supply to LCD Circuit

The power supply to the LCD screen should resemble the schematic shown above in order to meet the voltage and current requirements for input into the LCD. However, due to the incorporation of a backlight on the LCD, there may need to be another 9V battery added to the initial battery to meet the power requirements of the backlight. If need be, the 9V batteries could be put in parallel to ramp up the current to meet all of the current specifications.

Another important component of the handheld console will be the text-to-speech device. This device's incorporation into the design is vital to the user(s) that has extreme vision impairment or possible blindness. The group will be implementing the RC8650 Voice Synthesizer® Chipset made by RC Systems in order to accommodate the text-to-speech functionality. The RC8650 can store up to 3.5MB of memory and includes playback of fifteen minutes of pre-recorded messages. This is more than enough memory to include the speech output that is necessary for the device. The chip is available in 3.3V and 5V operating voltage packages, and the 5V operating voltage chip will most likely be chosen for the voltage specifications of the device. The RC8650 will connect to three ports on the microcontroller for input, output, and clear functionality. The RXD port of the chip will receive data (text) and commands from the microcontroller. The TXD port will be used to read information out of the RC8650, and CTS# port will acknowledge each byte received on the RXD pin by going high (it

is initially low) and allowing the data flow. The $A0_0$ and TS_0 pins will transmit the analog output and talk status output from the RC8650 to a low-pass filter operational amplifier circuit, which will then output to an 8 ohm speaker for audible speech output of the weight measurement to the user. Testing of the chipset will be done using a protoboard setup to connect a set of inputs to make sure that the outputs match the data and commands of the inputs. This can be done by setting up the RC8650 chipset testing circuit (given in the datasheet) on a protoboard to see if the DC characteristics match up to those provided in the datasheet. A figure showing a picture of the RC8650 chipset is shown below:

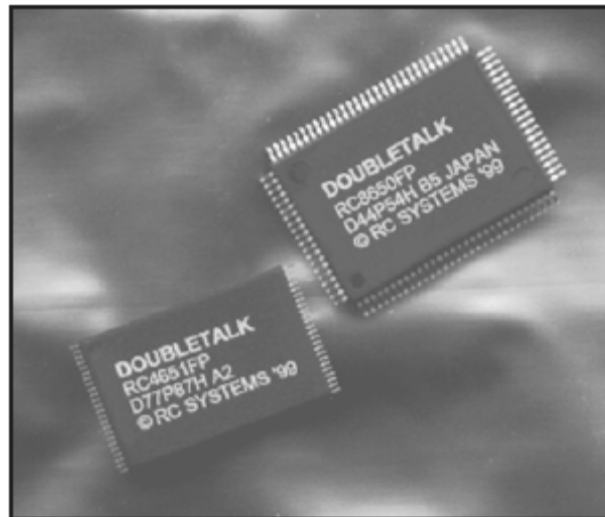


Figure 18 – RC8650 Chipset [5]

The outer casing of the console will be made of hard plastic. It will need to be big enough in size to safely fit the LCD, push buttons, batteries, and electrical components. Yet, it also must not be bulky in order to make it comfortable to the user. All of the buttons will be clearly labeled, either directly on the buttons or directly above or below the buttons. They will be labeled in English text as well as Braille for users with vision impairment. The “Measure” and “Tare” buttons will preferably be of the same size, but of different shapes and colors, making it even easier to distinguish between the two. The two arrow buttons will be the same size and color, but will be distinguished by the direction that they face (up/down, north/south). A number of push buttons were found that could be used in the design of the device; however, not many of the push buttons had an option to be bought with Braille incorporated into them. Grayhill Inc. is one manufacturer of push buttons that has an option for Braille on the push buttons, and an inquiry has been issued with them to see whether or not a word, such as “Measure”, can be put onto the push button. Innovation Industries Inc. is another company that actually manufactures push buttons with Braille already on them; however, these buttons are used for more commercial settings, like an elevator, and do not have Braille words on the push buttons that would be pertinent to the group’s device. Therefore, the best idea could be to purchase small “sticky sheets” of Braille words, such as “Measure” or “Tare”, which can then be put directly on the buttons.

As with the testing of the elevated toilet compartment circuitry, the handheld console circuitry will need to be tested on a protoboard. A standard smoke test will inevitably be

performed when powering on the electronics to make sure that all of the electrical components are functioning correctly and will function correctly when eventually connected to the PCB. A digital multi-meter will be used to check voltages, currents, and resistances throughout the protoboard to make sure that they meet the specifications of the various chip, LM317L, LCD, and buttons. This will also make sure that there are no short circuits throughout the circuit.

Similar to the third design the optimal design of the accessible weight scale for seated users will implement wireless/RF technology. The wireless/RF will help minimize the amount of exposed wires in the optimal design. A large wire from the elevated toilet compartment to the handheld console, containing power and input/output wires, would be exposed and subject to contact with water, which is a danger to the user and cannot exist in the design. Therefore, the LR Series Long Range Wireless Communication Modules, made by Linx Technologies, were chosen to meet the wireless/RF technology demands. The 418MHz transmitter and receiver modules were chosen, which will hopefully reduce the amount of interference during transmission and provide accurate transmission of data between the two PIC microprocessors. They can incorporate a supply voltage of 5V, which is good for the power systems of the design since 5V supplies will be used. The modules have a direct serial interface and that will allow for accurate communications between USART pins of the PIC microprocessors. The 10,000 bits per second data rate of the LS modules is more than enough for the transmission of the data needed for the project; yet this will result in quicker communication between the handheld console and elevated toilet compartment, thereby resulting in quicker visual and audible weight readings. No external components are needed for the wireless modules, except for an antenna; therefore, the 418Mhz CW Series antenna was chosen for receiving of the data in the 418MHz frequency. These antennas are fully weatherized, which is optimal due to the environment in which the antenna will be used.

2 Realistic Constraints

The realistic constraints of the accessible weight scale for seated users include engineering standards put forth by the Americans with Disabilities Act (ADA), the economic, health and safety, social, sustainability, and manufacturability constraints. All of these constraints were determined by the team and addressed in designing the optimal design of the accessible weight scale for seated users.

The most important engineering standard that should be met in the design of this project is the Americans with Disabilities Act (ADA) design standards for accessible design of water closets. The ADA is enforced by the Department of Justice of the United States. ADA was developed to protect the rights of Americans with disabilities. One ADA standard is that the handrails that will be used for this device have to have a diameter of 1-1/4 inches to 1-1/2 inches at the gripping site. The handrails have to be kept at least 1-1/2 inches from the wall. The handrail must not deform when a 250 pound bending stress or shear stress is applied to the handrail. Also the fastener or mounting device should be able to support a 250 pound lateral load or direct tension force. These are the only ADA requirements for this device. [7]

The economic constraints associated with this project will be the expense of the accessible weight scale for seated users. Our prototype costs cannot exceed \$2000. Our

projected cost for the optimal design prototype will be roughly \$1700. This leaves only \$300 cushion in the event one of the components is damaged during construction of the device. The future cost of the device is usually estimated as being 35% of the prototype costs making the device cost approximately \$600. The market price of the device will be higher in order to make a profit, but the price of the device should still be significantly lower than current products on the market. Many of the currently available products that meet our specifications of accuracy within one fifth of a pound and total capacity of 600 pounds cost between \$1,500 and \$2000. These designs are not incorporated into an elevated toilet seat and are less convenient for the user, but they set the standard for the price range of this device. In order to compete with these products, the accessible weight scale for seated users should be less expensive than the currently available products. Many public hospitals and would appreciate a less expensive accessible weight scale for seated users given their tight budgets. Also it may be more beneficial for hospitals or private owners to have the scale incorporated into an elevated toilet seat because it is one less device to purchase and cheaper than purchasing two separate devices.

There are some definite constraints to the device in regards to health and safety. Similar to any electronic device there is an inherent risk of electric shock to the user. Because the device will be housed in a bathroom setting, this risk is even greater due to regular contact with water. This means that all electrical components will have to be safely housed to prevent electrical shock to the user when the device comes into contact with water.

Also the device will have to be easy to sanitize in order to prevent the user from coming into contact with harmful bacteria. The device will be used as a toilet as well as a scale. It should be easy to sanitize between uses especially in a clinical setting. In building the device it will be important to make sure that there are no crevices or hard to clean regions that bacteria could grow.

Another health and safety constraint is making sure there are no sharp edges on the device that could potentially injure the user. Cuts sustained from sharp edges could be painful and if the surface is not clean they could also result in infection of the wound. Any sharp edges will have to be filed down until they are smooth. This is especially important with the posture support and the electrical component encasement part of the elevated toilet seat since these components will be built in the machine shop by the group members.

Another health and safety constraint is ensuring the stability of the elevated toilet seat on the toilet. Bathrooms are a common place for the mobility challenged to have a fall. The elevated toilet seat will have four stoppers that will hold the elevated toilet seat securely ensuring that it will not slide off of the toilet. Normal toilet seats have hinges to secure the toilet seat, but the elevated toilet seat will not.

A definite social constraint of this project is ensuring that the device will increase the quality of life for the clients. The main objective of biomedical engineering is to engineer solutions that will increase the quality of life. This means that the user should be able to independently use the device without the help of another person. By making the device easy to use for a mobility impaired individual, the device will better the quality of life for the individual, allowing them to have control of monitoring their weight themselves without feeling

embarrassed by a loved one seeing their weight or helping them use the device. Also it is important to make sure that the accessible weight scale does not prevent the user from using the toilet without the help of another person. This would significantly lower the quality of life of the user if they had to rely on another person to use the toilet if they did not previously have to do so.

Sustainability of the device is another constraint for this project. Most of the users are old and cannot be expected to repair the weight scale. The weight scale should require very little maintenance beyond sanitizing the device. The electrical and mechanical components should not in any way be subject to failure. This could be difficult because some of the users are obese and the scale will be exposed to substantial forces. Another concern for this device is that it should be capable of operating for a long period of time. The device should have a long battery life so that the user will not have to change the battery often and it should be easy for the user to change the battery when necessary. If the user has to dig through complicated wires in order to remove and replace the battery they will not replace the battery and the device will not work.

In the event that the accessible weight scale does need to be repaired, the device should be relatively easy to repair. The device should remain light weight so that it would not be too difficult for the users loved one to remove the device and bring it in for repairs. The posture support for this design is detachable, which will make it significantly easier to repair. Also the circuitry should be readily available. The top of the elevated toilet seat will have a removable panel to allow for easy access to the electrical components. The panel will be removed with a screwdriver to prevent the user from tampering with the electrical equipment and the inside of the of the component will have weather striping to prevent water from leaking in when the panel is in place.

One manufacturability constraint on this project is that the machine shop is not equipped with the machines required for working with plastics. This will drastically limit the choices of materials to be used for the accessible weight scale for seated users. Some of the materials might sacrifice aesthetics for functionality and manufacturability. When the actual device is manufactured there will be a greater number of machines available and the device may be produced with more aesthetically pleasing components.

3 Safety Issues

While designing this device it was important that the safety issues that are associated with the device were thought of, discussed and addressed within the design of the product. Many devices, especially electronic devices, have safety issues. These safety issues are not a problem for the user as long as they are properly addressed and accounted for in the design of the device. The different types of safety issues that have been determined for the accessible weight scale for seated users include electrical, biological and mechanical safety issues.

Any electronic device has an inherent possibility of causing electric shock to the user if constructed improperly. Electric shock is very dangerous and could cause pain, burns and even cardiac arrest. For this reason the accessible weight scale for seated users will be made water resistant. The elevated toilet design could come into contact with water on a regular basis and must not endanger the safety of the user while in contact with water. The accessible weight scale

will keep the wires and load cells from contact with water at all times. The handheld console will communicate with the rest of the device wirelessly so that there are no exposed wires.

Another potential safety issue associated with the accessible weight scale for seated users is sanitizing the device. The scale will be integrated into an elevated toilet seat and will be used as such. Especially in a clinical setting the scale may be used by multiple users and will come into contact with germs and bacteria that could be spread from user to user. It is important that the weight scale be easy to clean and sanitize in order to limit the amount of risk to the users. This means that the device should not have a large number of crevices and hard to clean areas that could house bacteria and increase the risk of the user coming into contact with harmful bacteria.

One of the mechanical safety issues associated with the accessible weight scale for seated users is the stability of the elevated toilet seat on the toilet. If the seat were to fall off the toilet with the user on it, it could cause considerable injury to the user. The elevated toilet seat is not as easy to stabilize on the toilet since it will not be attached to the toilet as a normal toilet seat is. It will not have a hinge attachment. It will, however, have the four fastening mechanisms installed at the four corners of the device to ensure the stability of the elevated toilet seat on the toilet. These mechanisms will hold the seat from any lateral movement and will resist vertical movement without inhibiting the load cells from compressing and measuring the force applied by the seated user.

Another mechanical issue associated with the optimal design is that it will have components built in the machine shop. It will be important to ensure that these components do not have any sharp metal edges that could injure the user. Any sharp edges will have to be filed down so that they are no longer sharp and no longer a danger to the user.

For each of the safety issues that have been determined for this project a solution has been made in order to ensure that the device is safe for the user. It will be important to keep these design solutions in mind while building the device. If it becomes apparent that one of the safety solutions is not adequate to keep the user safe a new solution will have to be developed or the old solution will have to be improved. The safety of the user is paramount to the success of the accessible weight scale for seated users.

4 Impact of Engineering Solutions

As engineers it is important to consider the impact of our engineering solutions prior to starting a project. It is the engineer's responsibility to ensure that their engineering solutions are ethical and beneficial to society. The impacts of the accessible weight scale for seated users include economic, societal, environmental, and global impacts.

There are two types of economic impact that the accessible weight scale for seated users would have. One type of economic impact would be the impact on the consumer, which would come in the form of a cheaper device. The second type of economic impact would be on the competing companies, which would come in the form of a competing device taking some of their market share.

By producing an accessible weight scale for seated users that is inexpensive, there will be an economic impact on the individual consumer. The individual consumer may have a fixed income, many expenses and limited savings. This consumer would save money by purchasing the accessible weight scale for seated users rather than purchasing other products that have the same capabilities, but are more expensive. The device would not only be cheaper, but it is an elevated toilet seat and weight scale combined. The consumer then only has to purchase this one device instead of spending more money by buying both a weight scale and an elevated toilet seat.

For competitors to the accessible weight scale for seated users the economic impact of the device will not be a good one. Competitors will have some of their market share taken by a less expensive and more convenient device. This means that competitors will lose money and be forced to drop prices in order to maintain their market share. They will also be forced to pour more money into research and development in order to design an accessible weight scale that is even better than their new competition. The companies' new products could be even cheaper and more convenient than the accessible weight scale for seated users, which will benefit the consumers. This benefit does not come to the consumers, however, unless new products are developed and introduced to the market.

The accessible weight scale for seated users could have a significant societal impact on people with limited mobility. It is currently quite difficult for seated users to monitor their weight. They often require another person's aid sometimes even having to travel to the hospital in order to measure their weight. This dependence on other people is sometimes very detrimental to the psyche of a mobility challenged person. They can often feel that they are a burden on their loved ones. This depression can be especially detrimental to obese patients with limited mobility because their depression could cause them to eat more and monitor their weight less. By developing a weight scale that is convenient and easy to use without the help of another person, it will be possible to increase the seated user's independence from their loved one. This will allow them to feel less of a burden and to let them focus on monitoring their weight and ensuring their continued health.

In order to ensure that this product is environmentally friendly the accessible weight scale for seated users will not use lead based materials to operate. Restriction of Hazardous Substances (RoHS) came into force on July 1 2006. This directive restricts the amount of lead, cadmium, mercury and other hazardous substances that can be contained in an electronic device sold in the European Union. In order to ensure that our device follows these standards, the electronic components for the accessible weight scale for seated users will only be purchased from RoHS compliant suppliers. In the event that the weight scale is thrown out it will not have as significant an impact on the environment as other electronic devices sometimes do. [7]

The design of the accessible weight scale for seated users can be easily adapted for a global market. It uses battery power and will not require power adaptors or power cords to work in different nations. Also the weight of the user is given in both pounds and kilograms, allowing users everywhere to clearly understand how much it is they weigh. Also this design will be RoHS compliant, meaning no lead based materials, which will allow the product to be sold in the European Union.

There are several factors that will impede the global impact of the accessible weight scale for seated users. One reason for this is that selling a product in an international market takes more time than selling the product in the United States. An international patent should be applied for in order to protect the device from being adopted and sold by other companies. Also international distribution channels would need to be fostered and grown. Before entering a market a significant amount of market research should be conducted. There may be products sold in foreign nations that have not yet made it to the United States. These products may already have a sizable piece of the market and depending on their design it may be difficult to take some of that market share with a new product. Also determining pricing strategies in foreign nations could take time given fluctuating values of foreign currency and a lower standard of healthcare and living in other nations. In the future these impedances may fall away, but for the time being the global impact of the accessible weight scale for seated users will be slow in coming.

Taking all of these impacts of engineering solutions for the accessible weight scale for seated users into account, there are many reasons to build this device and few reasons not to. The device will have negligible impact on the environment when compared with other devices and the economic impact is a positive one. The societal impact is the driving force for this project and is the main reason for developing this device. The users will benefit from being able to independently monitor their weight.

5 Life-Long Learning

Life-long learning is a concept that is present in educational institutions all over the world. The Australian department of education has defined life-long learning as “the process of acquiring knowledge or skills throughout life via education, training, work and general life experiences.” [8] The concept of life-long learning has made a large impact at the University of Connecticut. One of the program outcomes for the biomedical engineering program is, “a recognition of the need for, and an ability to engage in life-long learning.” [9] Our senior design project is a principle component of our education to meet this program outcome. In this project a number of skills have been developed through life-long learning that would not have been achieved through normal educational means. Among these skills are working on a multidisciplinary team, applying education in a real world application, learning market research concepts, and machine shop training.

In our educational experiences at the University of Connecticut each of the three team members have worked on several engineering projects. None of these projects have been as challenging and none of these projects have required that our teammates be from different tracks within the biomedical engineering program. The three tracks that are represented in our team are chemical engineering, bioinstrumentation and biomaterials.

The most important skill that is developed when working on a multidisciplinary team is delegating tasks. These projects are so large and time consuming that in order to complete them, tasks have to be delegated to the various team members in such a way that plays to their strengths based on previous experiences. Each team member could probably complete any of the

given tasks, but some are better than others because of their individual experiences at UConn. Determining which skills each person has and how best to implement those skills was probably the first challenge in this project and a skill that will be of great use in our careers.

The average engineering student has amassed a wealth of knowledge by their senior year of college, but may not have had many chances to apply that knowledge to real world problems. This is a skill that needs to be developed if the student is to succeed in his or her career. It is also a skill that is being developed in this senior design project. All of the seniors have to complete their senior design project in order to graduate with a degree in biomedical engineering from the University of Connecticut. Each team is asked to design a product that is needed in the world in order to increase the quality of life for their clients. In order to produce a successful project each team member has to apply the knowledge they have gained at UConn. Being able to apply that knowledge and skill is a lesson in and of itself.

These projects are all real world applications and that means that if it is going to be made for the real world it has to be able to be sold in the real world. This means that as engineers it is not acceptable to only develop a product that solves a problem. They must also develop a product that can compete in the market today. In order to do this it is necessary for the team to learn how to use market research in order to determine if there would be a market for their design project. The market research for these projects is limited to secondary research for the most part with the exception of the students who work on NSF projects and have a client with specific needs. For the rest it is imperative that they are able to see what other products are available and to design the project in a way that it can compete with the available products. This skill will inevitably be useful in future careers because it ensures that the product being engineered not only solves the problem, but can be sold as well.

Each senior design student is required to complete machine shop training. This training is necessary in order to ensure that the team can build the device in the second semester of senior design. This hands-on training is a skill that would not necessarily be learned at any other time in the student's life, but could be of definite benefit when working on future prototype designs at companies.

In each particular design it was important to come up with as many different creative innovations for each design. By making the designs as different as possible, a wider range of ideas were considered. In the optimal design it was important to sift through all of the previous design innovations and determine which of them are the best and should be included in the optimal design. This method and skill is something that will definitely be used again in future design groups. Being able to come up with as many creative ideas as possible and then being able to drill down and determine which of these creative ideas will work best for the product.

All of these additional skills that the student learns while completing their senior design project are important in meeting the program outcomes that the biomedical engineering program has developed. These program outcomes prepare the students for their future careers in the field of biotechnology and prepare them to continue their education through life-long learning.

6 References

- [1] National Instruments. <http://zone.ni.com/devzone/cda/tut/p/id/3642>
- [2] SMD Sensors. http://smdsensors.com/detail_pgs/s400.htm
- [3] ON Semiconductor Corp. <http://www.onsemi.com/pub/Collateral/LM317L-D.PDF>
- [4] Allied Electronics. <http://www.alliedelec.com/Search/ProductDetail.asp?SKU=670-1137&SEARCH=&ID=&DESC=LCM%2DS01602DSR%2FD&R=670%2D1137&sid=471550806480E17F#>
- [5] RC Systems. <http://www.rcsys.com/Downloads/rc8650.pdf>
- [6] “ADA Standards for Accessible Design,” Department of Justice, United States of America, available at, <http://www.usdoj.gov/crt/ada/adastd94.pdf>
- [7] RoHS “Home” <http://www.rohs.gov.uk/>
- [8] “Glossary of terms F to L” Department of Education, Science and Training Australian Government, available www.dest.gov.au/sectors/training_skills/policy_issues_reviews/key_issues/nts/glo/ftol.htm
- [9] “Program Outcomes,” Department of Biomedical Engineering, University of Connecticut, Storrs, CT, available at, <http://www.bme.uconn.edu/ugrad/bmeprgoc.htm>

Appendix A

Specifications

Performance		
Nonlinearity		< 0.1 % Rated Output (R.O.)
Hysteresis		< 0.05 % Rated Output (R.O.)
Nonrepeatability		< 0.03 % R.O.
Static Overload		
Safe		150 % Rated Capacity (R.C.)
Temp. Effect on Zero Balance		
Standard		< 0.038 % R.O. / °C
Temp. Effect on Output		
Standard		< 0.025 % Reading / °C
Body Material		17-4 PH stainless steel
<hr/>		
Electrical		
Rated Output (R.O.)		2 mV / V nominal
Excitation		
Recommended		10 Vdc
Maximum		15 Vdc
Bridge Configuration		Full Wheatstone Bridge
Bridge Resistance		350 ohms
Insulation Resistance		>1,000 MΩ @ 50Vdc
Electrical Termination		Shielded 28AWG 4C cable with drain wire, 24" long
<hr/>		
Mechanical	(Please order in	e.g. S400-250 lb)
lbs,		
Rated Capacity, Newtons		245, 445, 1,130, 2,255, 4,500
Rated Capacity, kg-force		25, 45, 115, 230, 460
Rated Capacity, lb-force		50, 100, 250, 500, 1,000

Appendix B

;;;;; ADConvert Subroutine ;;;;;;;;;;;;;;

ADConvert

```
    MOVLW    rdAN1    ;load appropriate control for RA1 input
    movlw d'15'    ;RP1 goes to RA1 on NEW #905172 education board
    movwf ADCHARGETIME
```

waitSet1

```
    decfsz  ADCHARGETIME,F    ;delay 30 usec for settling
    goto   waitSet1
```

```
    bsf    startAD          ;Start conversion
```

ADWait1

```
    btfsc  ADCON0,GO_DONE    ;check GO_DONE bit and continue if clear, i.e.
conv. complete
    goto   ADWait1
```

```
    call   BarTable          ;Convert ADRESH to port D coding
```

```
    movwf PORTD_CPY ;toggle returned bits into PORTD_CPY
```

```
    MOVLW    rdAN0          ;Select ADC's RA0/AN0 input
                                ;for intensity variable
```

```
    movlw d'15'
    movwf ADCHARGETIME
```

waitSet0

```
    decfsz  ADCHARGETIME,F    ;delay 30 usec for settling
    goto   waitSet0
```

```
    bsf    startAD          ;Start conversion
```

ADWait0

```
    btfsc  ADCON0,GO_DONE    ;check GO_DONE bit and continue if clear,
                                ;i.e. conv. complete
```

```
    goto   ADWait0
```

```
    MOVFF   ADRESH,TEMP2
```

```
    movlw  ADCON1 ;using indirect addressing
    movwf FSR ; right justify the AD converter
```

```

bsf    INDF,ADFM

MOVLF   rdAN3      ;Select ADC's RA3/AN3 input
                ;for intensity variable
movlw d'15'
movwf ADCHARGETIME
waitSet3
decfsz ADCHARGETIME,F      ;delay 30 usec for settling
goto   waitSet3

bsf    startAD      ;Start conversion

ADWait3
btfsc  ADCON0,GO_DONE      ;check GO_DONE bit and continue if clear,
                ;i.e. conv. complete
goto   ADWait3

movf   ADRESH,W      ;put high byte in T1HIGH
movwf  T1HIGH

movlw  ADRESL ;ADRESL is in bank 1, so must use
movwf  FSR ;indirect addressing to get it to
movf   INDF,W ;T1LOW
movwf  T1LOW

movlw  ADCON1 ;using indirect addressing
movwf  FSR ;right justify the AD converter
bcf    INDF,ADFM ;set back to left justify for other ADs

bcf    offAD      ;turn AD off, save energy

BarEnd
return

```

Appendix C

```
;;;;; InitLCD subroutine ;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;;
;
; Initialize the FEMA 16x2 character LCD display.
; (Initialize PIC ports prior to calling this subroutine.)
; This subroutine uses a one-byte RAM variable called LCD_TEMP.

InitLCD
    MOVLW    25,LCD_TEMP    ;Wait 1/4 second
InitLCD_1
    call    LoopTime    ;Call LoopTime 25 times
    decfsz LCD_TEMP,F
    goto    InitLCD_1
;LCD_TEMP now equals zero
    bcf    PORTE,0    ;RS=0 for command
InitLCD_2
    call    LCDinit_Table    ;Get next byte, pointed to by LCD_TEMP
    iorlw  H'00'    ;Set Z flag if W=0
    btfsc STATUS,Z
    goto    InitLCD_done
    movwf  TEMP_DISP    ;Save copy of byte
    swapf  TEMP_DISP,F    ;position for xfer part1
    rlf    TEMP_DISP,W    ;position for xfer part2

    movwf  PORTB    ;Send upper nibble
    bsf    PORTE,1    ;Drive E high
    bcf    PORTE,1    ;Drive E low so LCD will process input
    call   LoopTime    ;Wait ten milliseconds

    swapf  TEMP_DISP,F
    rlf    TEMP_DISP,W    ;rotate and put into W for Xfer
    movwf  PORTB    ;Send lower nibble
    bsf    PORTE,1    ;Drive E high
    bcf    PORTE,1    ;Drive E low so LCD will process input
    call   LoopTime    ;Wait ten milliseconds

    incf   LCD_TEMP,F;Point to next byte
    goto  InitLCD_2    ; and deal with it
InitLCD_done
    return
```

Appendix D

;;;;;; ScanKeys subroutine;;;;;;

ScanKeys

```
    MOVLW    TRISB,FSR
    movlw B'00011110'
    xorwf INDF,F;this sequence changes b1,2,3,4 to inputs
```

```
    clrf    KEYCODE    ;start by checking the "0" key
```

ScanKeys_1

```
    call    ScanKeys_Table    ;get next table entry
;;below xfers appropriate bits to columns
    movwf TEMPKEY; move to TEMPKEY for tests
```

```
    btfsc  TEMPKEY,3
    goto   SetCol1
    bcf    Col1
```

ChkCol2

```
    btfsc  TEMPKEY,2
    goto   SetCol2
    bcf    Col2
```

ChkCol3

```
    btfsc  TEMPKEY,1
    goto   SetCol3
    bcf    Col3
```

EndCol

```
    goto   TestRows
```

SetCol1

```
    bsf    Col1
    goto   ChkCol2
```

SetCol2

```
    bsf    Col2
    goto   ChkCol3
```

SetCol3

```
    bsf    Col3
    goto   EndCol
```

```
;; TestRows: compare B4,3,2,1 with table entry
```

```
;; keypressed->low->match->Z=1
```

TestRows

```
    swapf  TEMPKEY,F ;position for xfer part1
```

```

    rlf    TEMPKEY,W ;position for xfer part2
;;if a match, get all zeros in w1,2,3,4
    xorwf PORTB,W
;; AND screens so only compare RB1,2,3,4 inputs
;;Z=1 if a match, so return with value in KEYCODE
    andlw B'00011110'
    btfsc STATUS,Z
    goto  ScanKeys_done
    incf  KEYCODE,F ;otherwise try next key
;;stop with Z=0 when KEYCODE =xxxx1100
;;if both bits 3 and 2 set, will return [ScanKeys_done]
    btfss KEYCODE,3
    goto  ScanKeys_1

    btfss KEYCODE,2 ;stop with Z=0 when KEYCODE =xxxx1100
    goto  ScanKeys_1

```

ScanKeys_done

;;restore B1-4 to outputs

```

MOVLF    TRISB,FSR
bcf     INDF,1;change b1-b4 to output without
bcf     INDF,2 ;affecting z bit in status register
bcf     INDF,3 ;use indirect addressing
bcf     INDF,4

```

return